



Implementation of the Valco Helical Drive Air Actuator*

Two Position Valves

The recommended implementation approach for all Valco 2 position valves is to pulse a pair of 3-way solenoid valves (MSVA). This applies air to the actuator only during switching, and alleviates problems associated with continuous air pressure. The pulsed operation simulates switching by hand while providing the advantages of powered operation.

An air-actuated valve is often controlled by signals supplied by microprocessor-based instruments, data systems, or valve programmers. An interface such as Valco's Digital Valve Interface (DVI) can be used along with low-power negative true logic level signals or with data system contact closures.

PROCEDURE:

(Requires two external events.)

1. Energize solenoid A – valve rotor rotates clockwise. *A 2-second delay is recommended before the next step.*
2. De-energize solenoid – air pressure stops.
3. Energize solenoid B – valve rotor rotates counter-clockwise. *A 2-second delay is recommended before the next step.*
4. De-energize solenoid – air pressure stops.

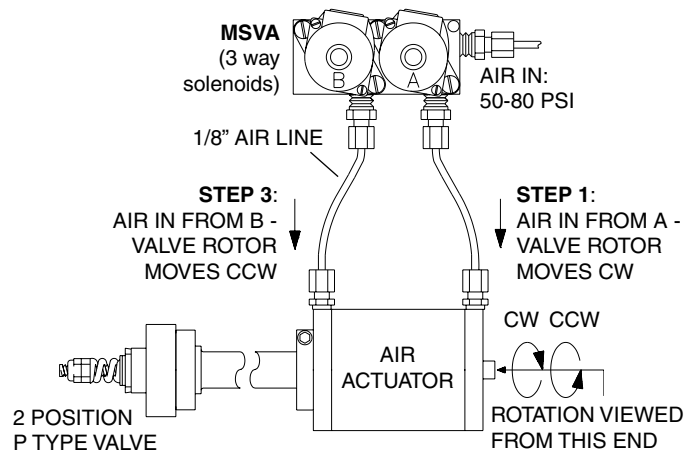


Figure 1

Recommended Actuator Air Pressure

CAUTION:

We recommend bottled instrument air or nitrogen. If plant air from a compressor must be used, an oil separator and water dryer are required.

The optimum actuator air pressure depends upon the type of valve in use. Beyond that, variances between like valves and actuators mean that some turn easier than others. General pressure ranges are indicated in the table below, but essentially the optimum pressure for any particular valve/actuator combination is that pressure which yields a reasonable switching time (nominally 0.5 seconds). In practice, it is better to err on the side of too much pressure rather than too little, but as the pressure increases so does the potential for problems associated with the optional 4-way operation described on the next page.

Valve type	Suggested air pressure
P	50-60 psi
UW	40-50 psi**
W	30-40 psi

**High pressure (2000-5000 psi UW valves may require 60-80 psi)

Alternate Implementation for 2 Position Valves

The use of two 3-way solenoid valves is the recommended implementation approach for all VICI two position valves. However, it is possible to use a single 41E1 4-way solenoid, as shown in **Figure 2**.

CAUTION:

When using the 41E1 4-way solenoid actuation, actuating pressure in excess of 60 psig may cause valve leakage.

PROCEDURE:

(Requires one external event.)

1. Energize solenoid – air in through Normally Closed port. Valve rotor rotates clockwise.
2. De-energize solenoid – air in through Normally Open port. Valve rotor rotates counterclockwise.

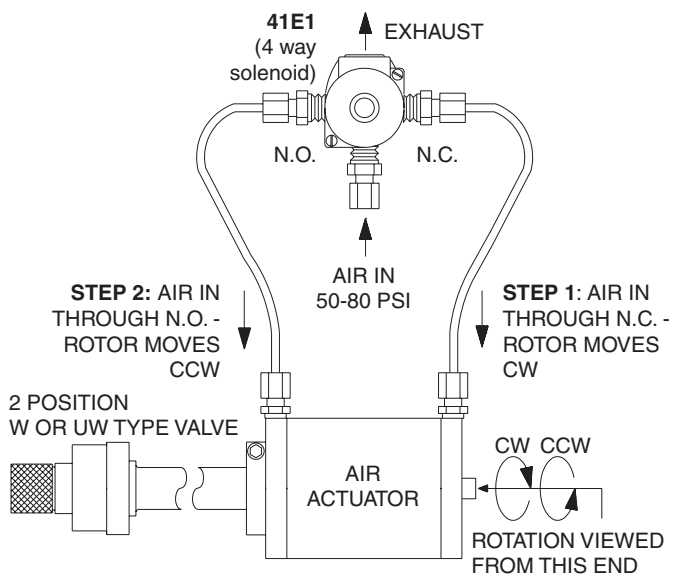


Figure 2

North America, South America, and Australia/Oceania contact:

VICI Valco Instruments Co. Inc.
P.O. Box 55603
Houston, TX 77255
Sales: (800) 367-8424
Tech: (713) 688-9345
Fax: (713) 688-8106 valco@vici.com

Europe, Asia, and Africa contact:

VICI VICI AG International
Parkstrasse 2
CH-6214 Schenkon
Switzerland
Phone: +41 41 925 6200
Fax: +41 41 925 6201 info@vici.ch

Cheminert® and VICI® are registered trademarks of Valco Instruments Co. Inc. and VICI AG

TN-405 Rev 7/18